




23010 N. 19th Ave  
Bldg 2 - Ste 48  
Phoenix, AZ 85065  
1-800-243-0820

### Custom Product Design Information Cradle with Extender

Company


Contact Name

Phone/Email

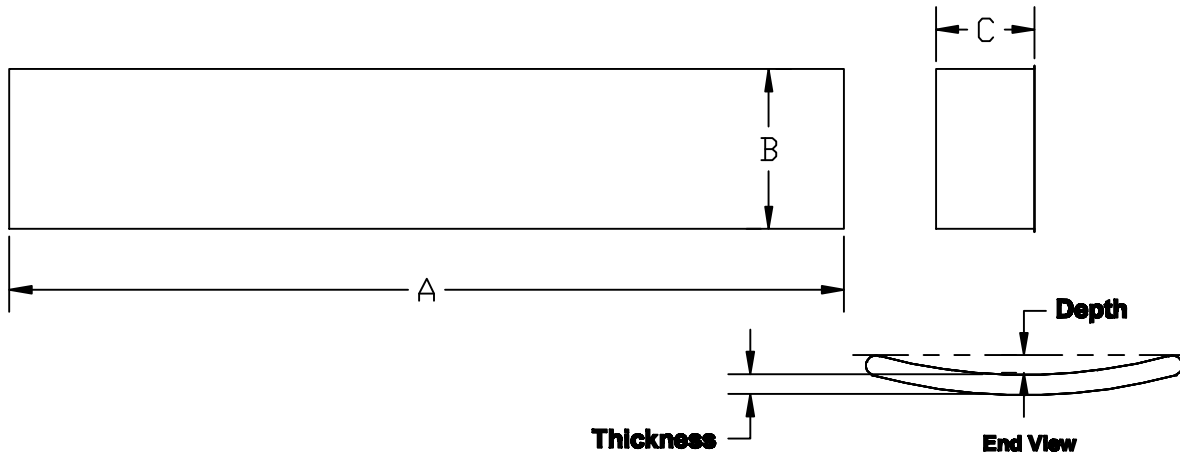

Please measure your pad/cushion at each lettered position shown in the illustration. Write the measures in the Table of Measures provided below

Table of Measures	
Letter	Measure (Inch or cm)
A	
B	
C	
Depth	
Thickness	



If your pad/cushion fastens to the table using Hook and Loop fastener (i.e. Velcro®), or other methods, please use the illustration to the left to sketch the locations and the measures of their position. Also, if the shape of the ends are not square, please sketch the shape on the illustration.

Please return this completed form to RadScan Medical Equipment, Inc. at:  
Fax: 623-580-0115  
Email: [orders@radscanmedical.com](mailto:orders@radscanmedical.com)